



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Southern Star Farm/Amber Adams
Rt 1, Box 79B
Alexander City AL 35010 USA

07/24/08

Test No: 329907


Animal and Sample Description

Animal Name: SSFA Buckshot
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt. Fawn

Animal ID: 30502413
Sample Location: Blanket
Sample Date: 05/12/08
Age: 05/14/07

Laboratory Data

Mean Fiber Diameter:	21.0 microns	Spin Fineness:	19.7 microns
Standard Deviation:	3.4 microns	Mean Curvature (deg/mm):	32.8
Coefficient of Variation:	16.1 %	SD Curvature (deg/mm):	21.4
Fibers Greater Than 30 microns:	1.2 %		
Medullated Fibers:	4.0 %		

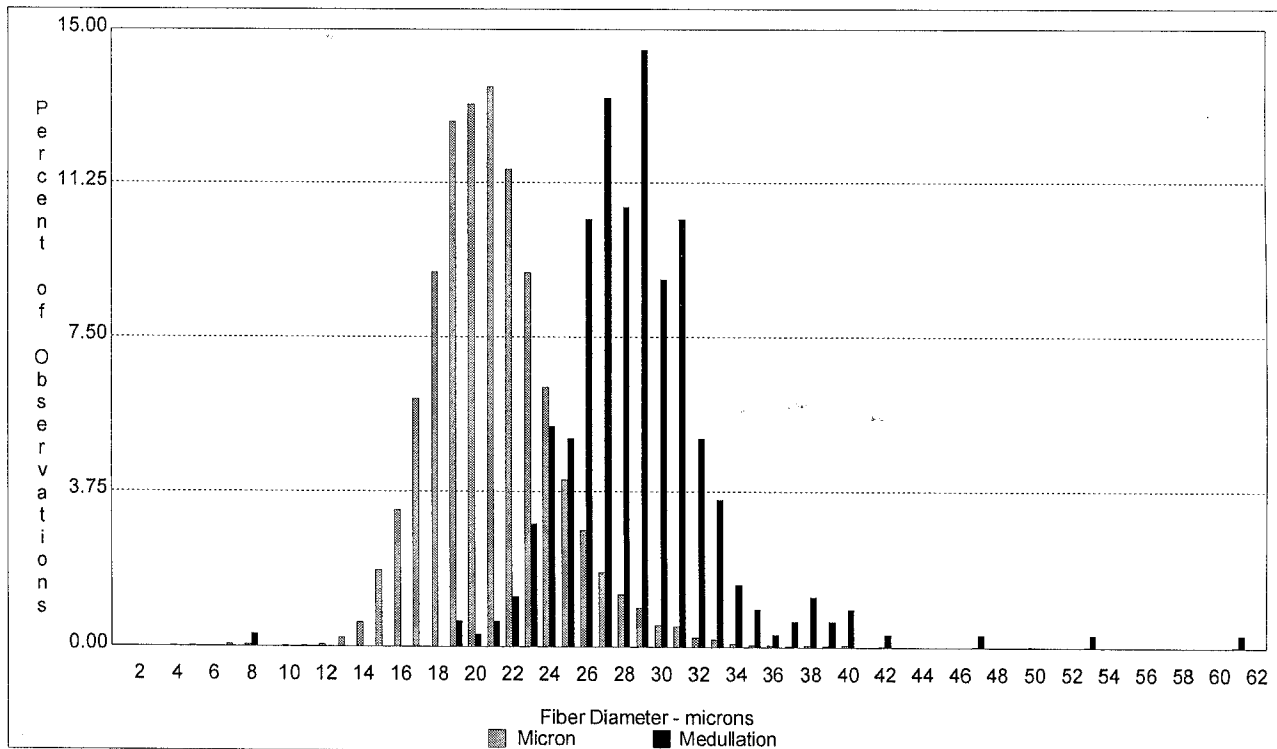

This Test Performed According to I.W.T.O Method 47