

## Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

### Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Southern Star Farm/Amber Adams  
Rt 1, Box 79B  
Alexander City AL 35010 USA

07/24/08

Test No: 32990


#### Animal and Sample Description

**Animal Name:** SSFA's Delaney  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** True Black

**Animal ID:** 30502284  
**Sample Location:** Blanket  
**Sample Date:** 05/12/08  
**Age:** 06/19/07

#### Laboratory Data

<b>Mean Fiber Diameter:</b>	21.4 microns	<b>Spin Fineness:</b>	20.7 microns
<b>Standard Deviation:</b>	4.4 microns	<b>Mean Curvature (deg/mm):</b>	37.0
<b>Coefficient of Variation:</b>	20.4 %	<b>SD Curvature (deg/mm):</b>	21.4
<b>Fibers Greater Than 30 microns:</b>	3.6 %		

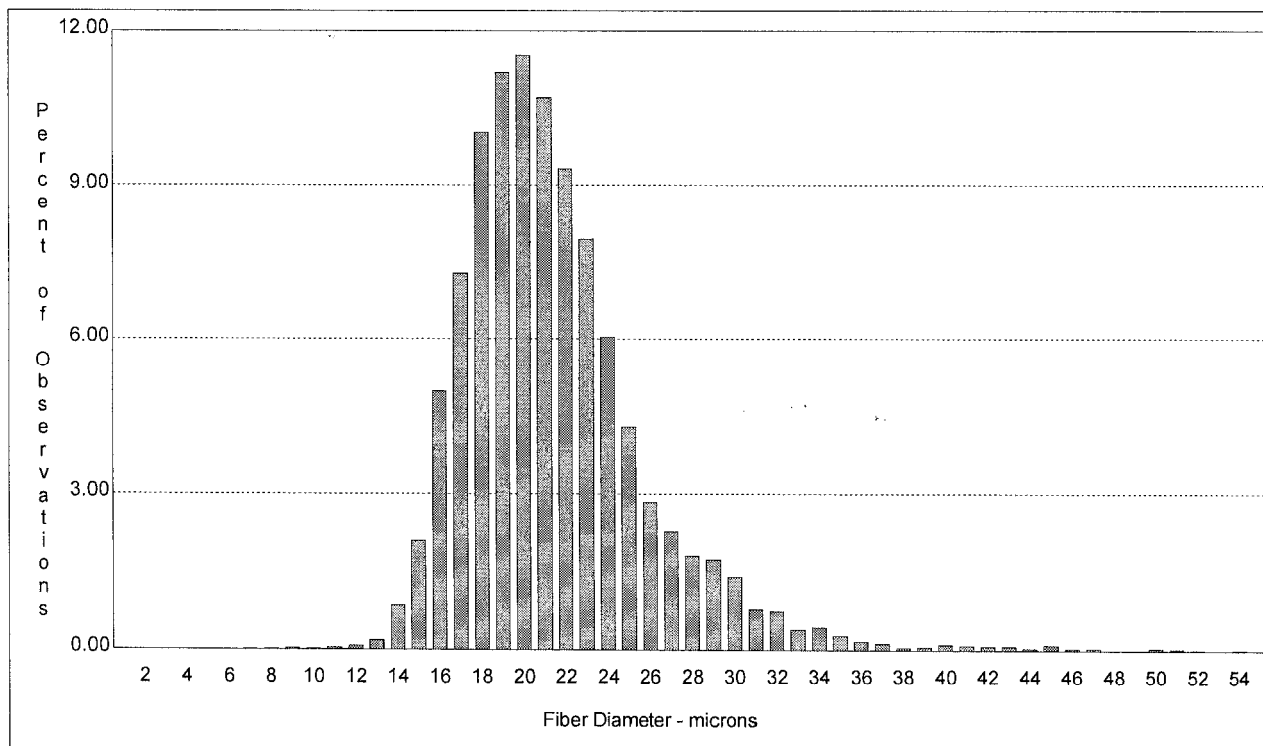

This Test Performed According to I.W.T.O Method 47