

**Yocom-McColl Testing Laboratories, Inc.**  
 540 West Elk Place • Denver, Colorado 80216-1823 USA  
 PHONE (303) 294-0582 • FAX (303) 295-6944  
 EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)  
 Micron Test Report**

Southern Star Farm/Amber Adams  
 Rt 1, Box 79B  
 Alexander City AL 35010 USA

07/24/08


**Test No:** 329894

**Animal and Sample Description**

<b>Animal Name:</b> Leah	<b>Animal ID:</b> 827972
<b>Breed:</b> Alpaca(Huacaya)	<b>Sample Location:</b> Blanket
<b>Sex:</b> Female	<b>Sample Date:</b> 05/12/08
<b>Color:</b> True Black	<b>Age:</b> 06/28/00

**Laboratory Data**

<b>Mean Fiber Diameter:</b> 33.0 microns	<b>Spin Fineness:</b> 31.7 microns
<b>Standard Deviation:</b> 6.4 microns	<b>Mean Curvature (deg/mm):</b> 26.1
<b>Coefficient of Variation:</b> 19.3 %	<b>SD Curvature (deg/mm):</b> 16.1
<b>Fibers Greater Than 30 microns:</b> 62.4 %	

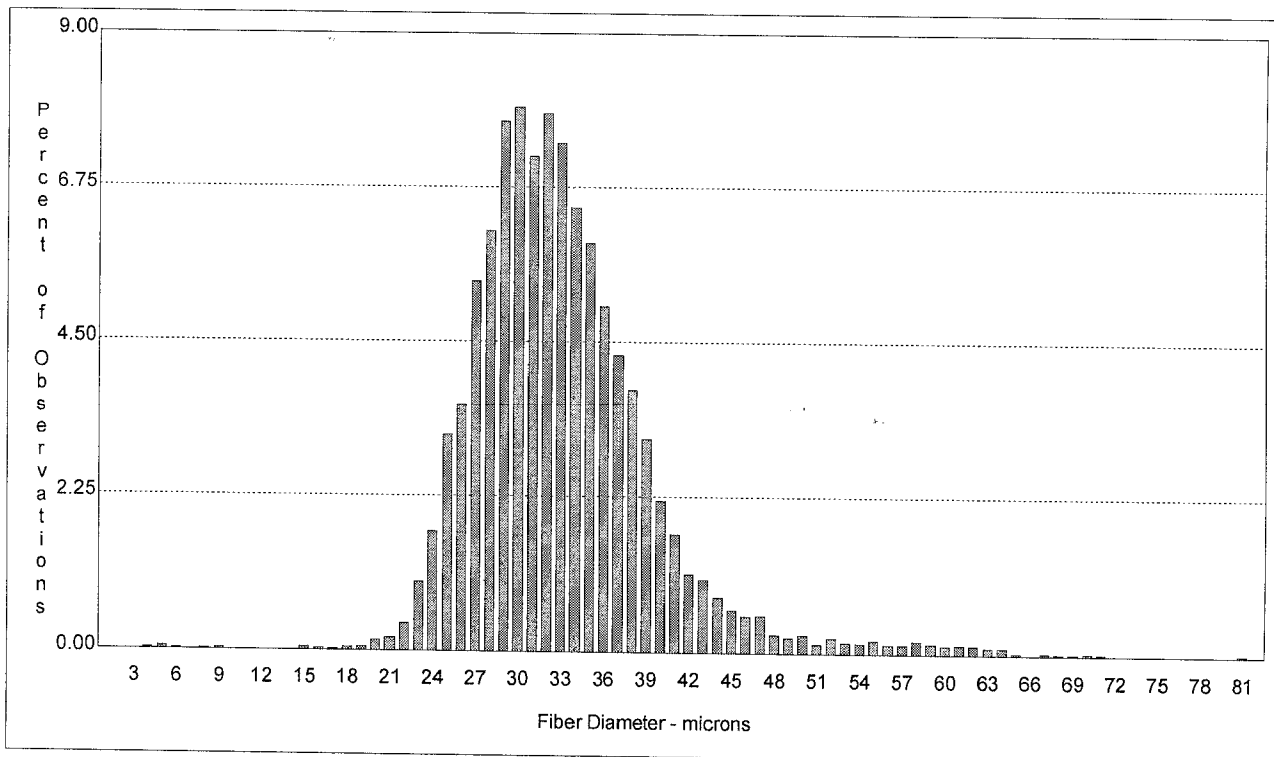

**This Test Performed According to I.W.T.O Method 47**