

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Southern Star Farm/Amber Adams
Rt 1, Box 79B
Alexander City AL 35010 USA

07/24/

Test No: 329


Animal and Sample Description

Animal Name: Noel
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Fawn

Animal ID: XXXXX
Sample Location: Blanket
Sample Date: 05/12/08
Age: 12/15/07

Laboratory Data

Mean Fiber Diameter:	23.2 microns	Spin Fineness:	22.2 micrc
Standard Deviation:	4.3 microns	Mean Curvature (deg/mm):	31.6
Coefficient of Variation:	18.7 %	SD Curvature (deg/mm):	19.3
Fibers Greater Than 30 microns:	4.0 %		

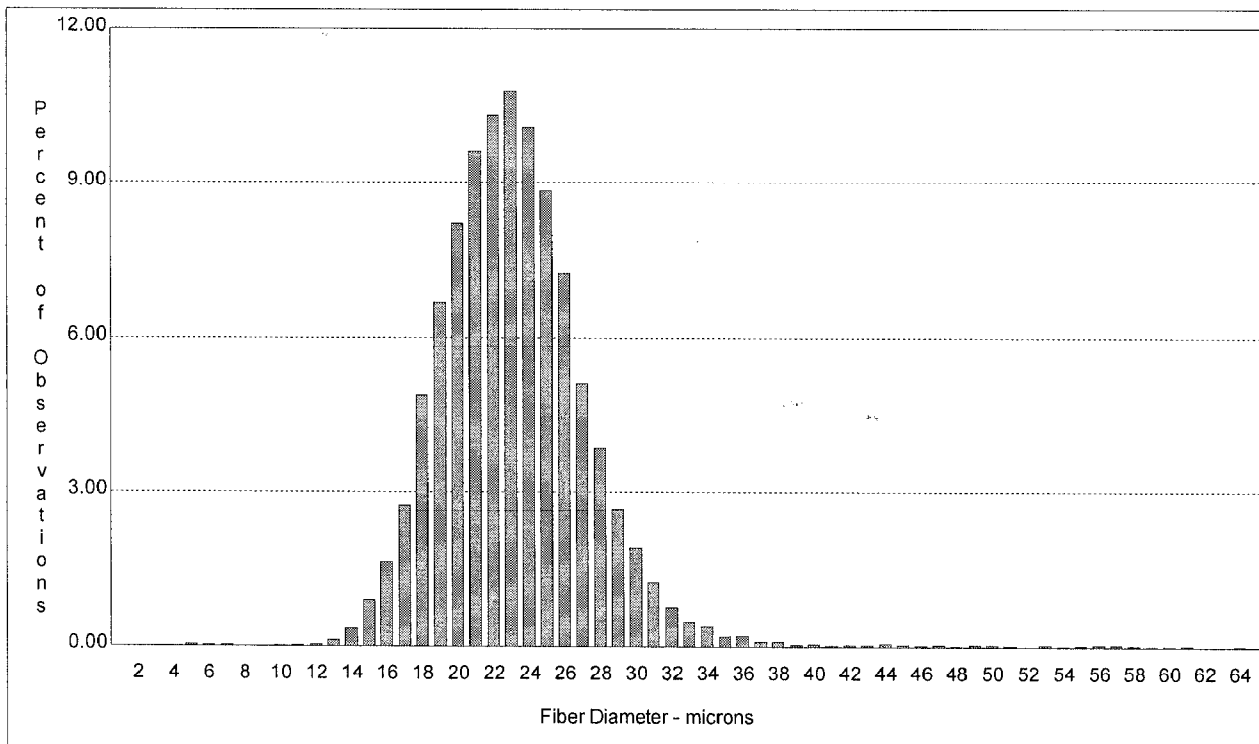

This Test Performed According to I.W.T.O Method 47