



**Yocom-McColl Testing Laboratories, Inc.**  
540 West Elk Place • Denver, Colorado 80216-1823 USA  
PHONE (303) 294-0582 • FAX (303) 295-6944  
EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)  
Micron Test Report**

Southern Star Farm/Amber Adams  
Rt 1, Box 79B  
Alexander City AL 35010 USA

07/24

**Test No:** 32


**Animal and Sample Description**

**Animal Name:** Pamela Lagos  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Med. Brown

**Animal ID:** 171209  
**Sample Location:** Blanket  
**Sample Date:** 05/12/08  
**Age:** 01/01/94

**Laboratory Data**

<b>Mean Fiber Diameter:</b>	28.6 microns	<b>Spin Fineness:</b>	28.2 micr
<b>Standard Deviation:</b>	6.5 microns	<b>Mean Curvature (deg/mm):</b>	27.0
<b>Coefficient of Variation:</b>	22.6 %	<b>SD Curvature (deg/mm):</b>	18.7
<b>Fibers Greater Than 30 microns:</b>	26.6 %		

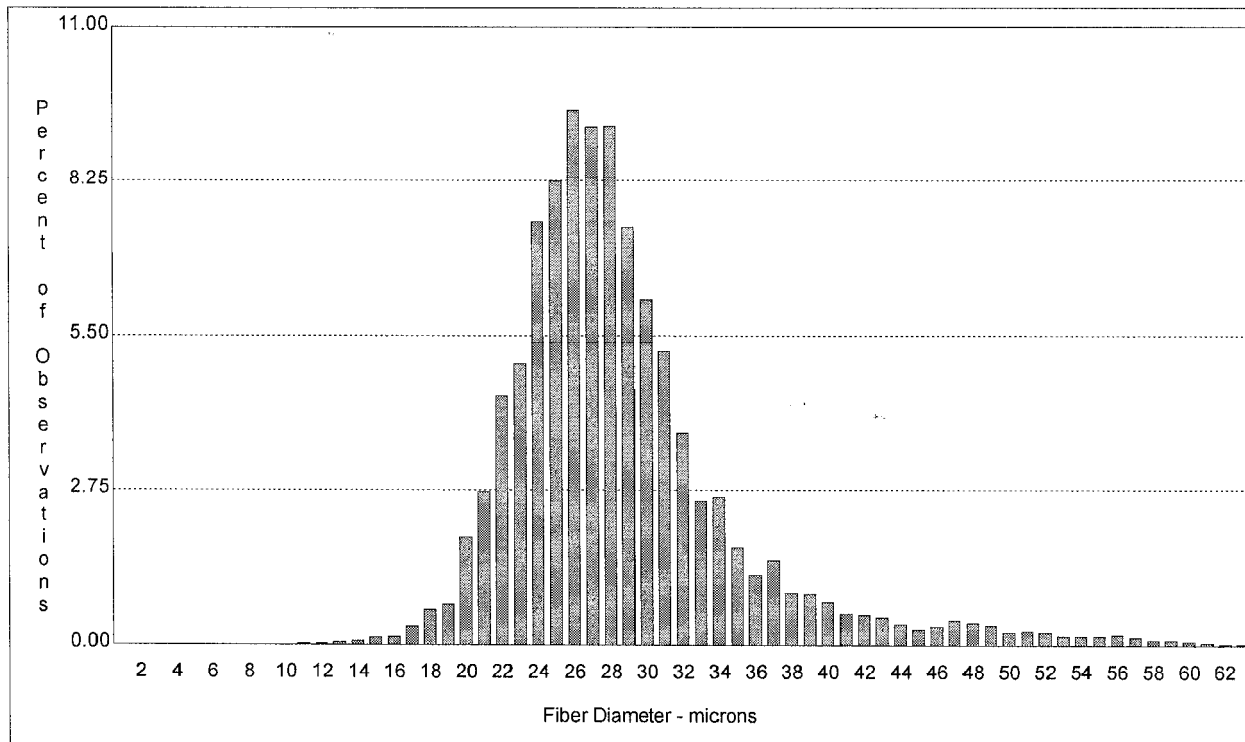

**This Test Performed According to I.W.T.O Method 47**