

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Southern Star Farm/Amber Adams  
Rt 1, Box 79B  
Alexander City AL 35010 USA

07/24/08

Test No: 329906


### Animal and Sample Description

Animal Name: SSFA Peruvian Autumn Skye  
Breed: Alpaca(Huacaya)  
Sex: Female  
Color: Med. Fawn

Animal ID: 1272277  
Sample Location: Blanket  
Sample Date: 05/12/08  
Age: 11/09/05

### Laboratory Data

Mean Fiber Diameter:	19.7 microns	Spin Fineness:	19.0 microns
Standard Deviation:	3.9 microns	Mean Curvature (deg/mm):	44.4
Coefficient of Variation:	20.0 %	SD Curvature (deg/mm):	25.9
Fibers Greater Than 30 microns:	1.2 %		

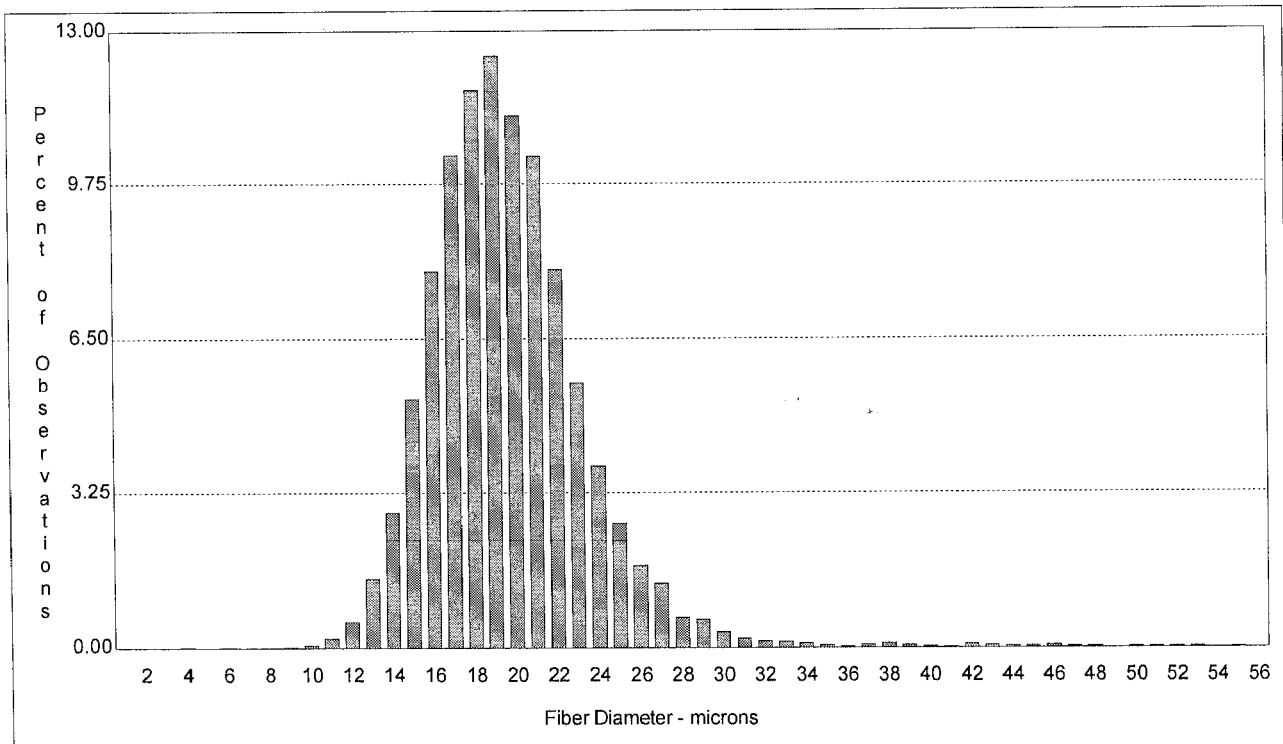

This Test Performed According to I.W.T.O Method 47